

# Development and Assessment of Measuring/Rehabilitation Device for Myelopathy Patients with Lower Extremity Function

Hironobu Murayama, Shohei Shimizu, Masakazu Ohnuki, Hisanori Mihara, and Tohru Kanada

**Abstract**—Disordered function of maniphalanx and difficulty with ambulation will occur insofar as a human has a failure in the spinal marrow. Cervical spondylotic myelopathy as one of the myelopathy emanates from not only external factors but also increased age. In addition, the diacrisis is difficult since cervical spondylotic myelopathy is evaluated by a doctor's neurological remark and imaging findings. As a quantitative method for measuring the degree of disability, hand-operated triangle step test (for short, TST) has formulated. In this research, a full automatic triangle step counter apparatus is designed and developed to measure the degree of disability in an accurate fashion according to the principle of TST. The step counter apparatus whose shape is a low triangle pole displays the number of stepping upon each corner. Furthermore, the apparatus has two modes of operation. Namely, one is for measuring the degree of disability and the other for rehabilitation exercise. In terms of usefulness, clinical practice should be executed before too long.

**Keywords**—Cervical spondylotic myelopathy, disorder of lower limbs, measuring function, rehabilitation function, full automatic apparatus, triangle step test.

## I. INTRODUCTION

THE aim of this research is to develop a full automatic and accurate apparatus for myelopathy patient in the measurement of the degree of disability.

### A. Myelopathy

The cause of myelopathy is that the spinal marrow in the spinal canal is compressed by bone deformation due to increased age and external compression to the spine. The myelopathy is a neurologic disorder in spinal marrow or brain, and sets up a disorder of upper motor neuron. Then, paralysis and painful in upper and lower limbs will come out, and may induce disorders of defecation and urination [1].

H. Murayama is with the Graduate School of Engineering, Kanto Gakuin University, 1-50-1 Mitsuura-higashi, Kanazawa-ku, Yokohama 236-8501, Japan (e-mail: m1141011@kanto-gakuin.ac.jp).

S. Shimizu is with the College of Engineering, Kanto Gakuin University, 1-50-1 Mitsuura-higashi, Kanazawa-ku, Yokohama 236-8501, Japan (e-mail: f0941066@kanto-gakuin.ac.jp).

M. Ohnuki is with the College of Engineering, Kanto Gakuin University, 1-50-1 Mitsuura-higashi, Kanazawa-ku, Yokohama 236-8501, Japan (e-mail: oonuki@kanto-gakuin.ac.jp).

H. Mihara is with the Division of Spine Surgery, Department of Orthopaedic Surgery, Yokohama Minami Kyosai Hospital, 1-21-1 Mitsuura-higashi, Kanazawa-ku, Yokohama 236-0037, Japan (e-mail: hmihara@ruby.ocn.ne.jp).

T. Kanada is with the College of Engineering, Kanto Gakuin University, 1-50-1 Mitsuura-higashi, Kanazawa-ku, Yokohama 236-8501, Japan (corresponding author to provide phone and fax: +81 45 786 7111; e-mail: kanada@kanto-gakuin.ac.jp).

Facing with such frame, the authors focused attention on cervical spondylotic myelopathy which is one of the possible medical problems whose possibility is relatively high. Generally, clinical condition of cervical spondylotic myelopathy is comprehended coupled with neurologic remark and imaging findings. However, for understanding accurately the functional disability owing to the damage to the spinal cord, doctor's neurological remark has limitations in objective and quantitative evaluation. Additionally, the neurological remark may not coincide with imaging findings [2]. As one of the improvement plans for such current reality, noninvasive and quantitative procedure has been newly established to evaluate the degree of disturbance of motor function in maniphalanx and lower extremities (ambulation).

### B. Triangle Step Test (TST)

One of the authors has been developed a method for measuring the degree of disability in disturbance of motor function, which is called 'triangle step test' (for short, TST). Then the method is applied in clinical practice. As shown in Fig. 1, a thin regular triangle board, whose three corners are painted in black, is placed in front of a patient sitting in a chair. The length of a side is 30cm. The patient steps the painted corners in sequence for a given length of time (usually 10 second). A surveyor counts the number of steps by visual judgment to evaluate the degree of disability. By means of TST, the obtained quantitative result has a certain correlation with Nurick scale and JOA score. Here, Nurick scale is a typical guidepost for Myelopathy and JOA score is a criterion for treatment results for myelopathy defined by the Japanese Orthopaedic Association. Therefore, we can say that TST is a safe and easy procedure, but it depends on visual judgment [3].

However, in the simplified measuring technique using a triangle board, the stepping force to the triangle board is not detected. Therefore, a patient intends to let the sole slide quickly on the board in order to increase the number of steps. This thing may lead to doubtful result for judging the degree of disability and deficiency in assuredness.

Thus the authors deal with a design and development of a prototype of full automatic and accurate step counter apparatus, by which the functional evaluation based on TST and additional rehabilitation exercise of motion in lower limb can be performed.

The step counter apparatus consists of a stepstool (triangle step board; for short, TSB) and a processing box (for short, PB).

In what follows further details about the step counter apparatus are described.

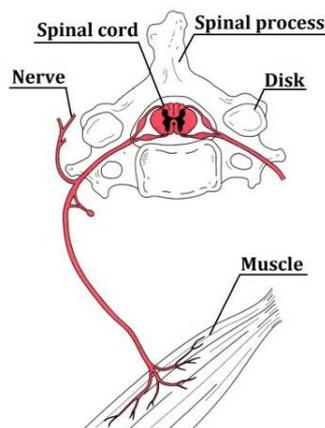


Fig. 1 Detail view of the spinal cord




Fig. 2 Regular triangular board applied for TST

TABLE I  
 NURICK SCALE

Grade	Severity (Degree of disability)
0	Signs or symptoms of root involvement but without evidence of spinal cord disease
1	Signs of spinal cord disease but no difficulty in walking
2	Slight difficulty in walking that does not prevent full-time employment
3	Difficulty in walking that prevents full-time employment or the ability to perform housework, but that is not severe enough to require someone else's help to walk
4	Able to walk with someone else's help or the with aid of a frame
5	Chair bound or bedridden

TABLE II  
 JOA SCORE FOR CERVICAL MYELOPATHY  
 (DISABILITY SCALE FOR LOWER EXTREMITIES)

Grade	Severity (Degree of disability)
0	Unable to walk
1	Can walk on flat floor with walking aid
2	Can walk up and/or down stairs with handrail
3	Can walk up and/or down stairs with handrail
4	Lack of stability and smooth gait
5	No difficulties

## II. STRUCTURE OF APPARATUS DEVELOPED

In this study, the step counter divides into two devices, developed separately. One is "Triangle Step Board(TSB)" as a device to step. The other is "Processing box (PB)".

### A. Triangle Step Board(TSB)

Fig. 3 represents a picture of the developed TSB.

In each corner of the TSB, a regular triangle plate, 10cm on a side, tilts with a mechanism of hinge and spring. A pressure-sensitive sensor is allocated under the plate. Thus existence or nonexistence of stepping force is detected when a patient steps on the plate on the corner. Furthermore, directly-aligned LEDs along the side of triangle board are lighting-up to indicate the circling direction which means the stepping sequence. The circling direction can be changed by a selecting switch arranged in the lateral side of the TSB.

A double-digit seven-segments LED allocated at a nearby site of each corner displays a number of stepping on relevant plate on the corner. In addition, a triple-digit seven-segments LED displays a total number of stepping to all plates on three corners. This is, so-called, an up-counter. Such number count is executed for a given length of time (usually 10 s [2]). The length of time can be given by a triple-digit BCD switch, arranged in the lateral side of the TSB, between 0 to 999 second. Remaining time is displayed on the triple-digit seven-segments LED allocated near the center of TSB. This is, so-called, a countdown timer.

The above-mentioned function can be performed in a measurement mode and a buzzer sound plays at the same moment of stepping on each plate of TSB.

A mode select switch is also allocated in the lateral side of the TSB. By this switch, two performance modes can be selected. Namely, one is a mode for measurement of the degree of disability and the other for rehabilitation exercise. In the rehabilitation exercise mode, a patient can try to step the plates in tune with the buzzer sound played at a constant frequency. The constant period in 0.01 second can be set by a triple-digit BCD switch arranged in the lateral side of the TSB. Moreover, the performance time in 0.01 second is displayed (as a countdown timer) on another triple-digit seven-segments LED allocated near the center of TSB. The authors expect this function to have a beneficial effect on rehabilitation treatment.

### B. Processing Box (PB)

Fig. 4 shows the controller. The controller consists of three substrates are classified into a power supply unit, a timer unit, a counting unit, respectively.

Further details about the above-mentioned (2) and (3) circuits are described later.

### C. Pressure-Sensitive Sensor

A pressure-sensitive sensor whose trade name is Inastomer ® (made by Inaba Rubber Co., Ltd.) is applied in this development. Fig. 5(a) and 5(b) represent a specification of Inastomer and detecting principle, respectively. Basically, Inastomer is made from an Inastomer chip, resin film and flexible foundation (lead film tracks). Inastomer chip is produced from conductive rubber material (elastomer).

As shown in Fig. 5(b), the conductive materials do not make contact with each other and the resistance between the leads is infinite (insulator) when no force (load) is applied. Then, the resistance value decreased with increasing applied force. In

other words, the relationship between the contacting area between conductive materials occurred by the applied force and the resistance value is in inverse proportion [4]. Therefore, when a force above a certain level is loaded, the apparatus recognizes existence of stepping on the corner plate of TSB.

Furthermore, threshold-based evaluation of the degree of disability may be capable by means of changing the threshold level for the resistance value.



Fig. 3 Triangle Step Board(TSB)



Fig. 4 Processing box(PB)

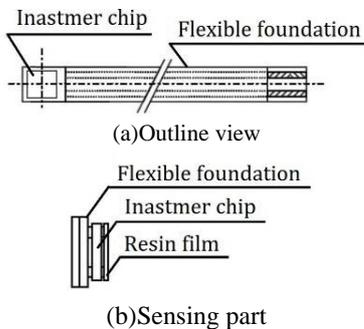


Fig. 5 Inastmer®

### III. FUNCTION OF ELECTRICAL CIRCUITS

This system has two modes which are measuring mode and

guidance mode. A signal from a pressure-sensitive sensor is processed by threshold. When the stepping force is large and the pressure-sensitive sensor signal exceeds the threshold, a pulse signal is generated.

In the measuring mode, once a pulse signal is generated from any one of three stepping points, a countdown timer begins to tick from an initial setting time (typically, 10 second) fixe by triple digits BCD switches. Then, the numbers of steps of each stepping point and total number of steps are displayed by seven-segments LEDs. When the measuring time comes to an end, the function for counting the number of steps terminates. In addition, a buzzer sounds at the same time by the abovementioned pulse signal.

In the guidance mode, regardless of existence or nonexistence of stepping, a buzzer sounds at regular intervals (0.01 second to 9.99 second) fixed by triple digits BCD switches. A patient gives exercise to step the TSB in tune with the buzzer sound in order to improve the degree of disability. As a matter of course, the number of steps is displayed in the same fashion of measuring mode.

Fig. 6 represents schematic illustration of the circuit developed.

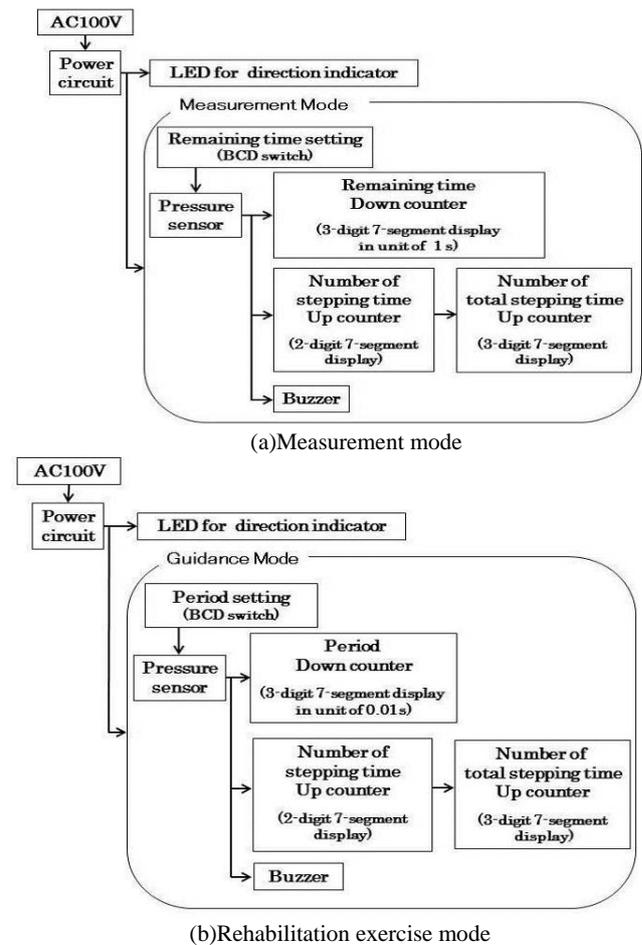


Fig. 6 Structure of electrical circuit



(a) TSB and PB



(b) Appearance of stepping number count and countdown timer




(c) Clinical usage

Fig. 7 Photographs of experimental verification

#### IV. VERIFICATION EXPERIMENT

The functions of this full automatic and accurate step counter apparatus were confirmed. In other words, response of pressure-sensitive sensor (Inastmer), display of all seven-segments LEDs were correct as expected. Fig. 7 represents the appearance of verification experiment.

What is troubling is that there are too many conducting wires between TSB and PB and mechanistic weak point arising from step vibration.

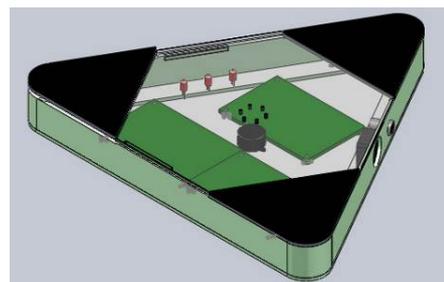

(a) TSB for second prototype



(b) PB for second prototype

Fig. 8 Second prototype to be developed

#### V. CONCLUSION

In this research, a full automatic and accurate measuring/rehabilitation exercise apparatus has been developed to evaluate the degree of disturbance of motor function in lower limb for myelopathy patient. Then the functions of the prototype were verified.

To confirm the reliability and durability, clinical experiment is proposed at some early date.

Moreover, since the height, 45mm of this first prototype is comparatively thick and the practical usefulness is slim, a second prototype is designed to upgrade the practical utility. In addition, timer and number count displays will be moved to the front panel of processing box in order to check the counted results easily by both surveyor and patient.

Fig. 8 represents an image of the second prototype to be developed. The first prototype has been used for real clinical usage in Yokohama Minami Kyosai Hospital. Some mechanical defects are reported and they have been fixed. In the second prototype, the stepping mechanism is improved and the seven-segment LEDs are replaced from TSB to the front panel of PB. Thus, the number of connecting wires between TSB and PB are greatly reduced.

#### REFERENCES

- [1] David J. Magee, "Orthopedic Physical Assessment, Fourth Edition," Elsevier Japan, 2006, pp.111-162.
- [2] S. Kobayashi, "Electrodiagnosis of the Spinal Cord Using the Motor Evoked Potentials and Short Latency Somatosensory Potentials in Patients with Cervical Myelopathy," Journal of the Kyorin Medical Society, 1999, vol. 30, pp. 223-230.
- [3] H. Mihara, S. Kondo, J. Murata, W. Ishida, T. Niimura, "A new assessment method for lower extremity function in myelopathy patients: triangle step test," The Journal of the Japanese Society for Spine Surgery and Related Research, 2008, vol.19, pp. 520-23.
- [4] M. Uehara, S. Fukuda, S. Nakata, A. Nakashima, "A study on the relationship between occlusal pressure distribution and maxillofacial morphology in adult subjects with normal occlusion," Journal of the Japanese Orthodontic Society, 2000, vol.59, pp.98-110.